

# Instructions for Use and Technical Description

# **Passive Mattresses**

EffectaCare 20

EffectaCare 20 B

EffectaCare 20 P

**PrimaCare 10** 

PrimaCare 20

PrimaCare 20 B

CliniCare 10

CliniCare 10 P

CliniCare 20

CliniCare 30



D9U004PPM-0101

Version: 01

Publication Date: 2021-04



#### Manufacturer:

LINET spol. s r.o. Želevčice 5 274 01 Slaný

Tel.: +420 312 576 111 Fax: +420 312 522 668

E-mail: info@linet.cz http://www.linet.com

Service department: service@linetgroup.com

#### **Passive Mattresses**

EffectaCare 20 B
EffectaCare 20 P
PrimaCare 10
PrimaCare 20 P
PrimaCare 20
PrimaCare 20 B
CliniCare 10
CliniCare 10 P
CliniCare 20
CliniCare 30

Author: LINET, s.r.o. Related links: www.linet.com

#### D9U004PPM-0101

Version: 01

Publication Date: 2021-04

Copyright © LINET, s.r.o., 2021 Translation © LINET, 2021 All rights reserved.

All trademarks and brands are the property of the appropriate owners. The manufacturer reserves the right to changes in the contents of the instructions for use that relate to the product's technical regulations. It is for this reason that the contents of the instructions for use may indicate differences from the current manufacture of the product. Reproduction, also excerpts, only with prior permission of the publisher. Subject to changes due to technical developments. All technical data are rated data and are subject to construction and manufacturing tolerances.



# **Table of Contents**

1 Symbols and Definitions	
1.1 Warning Notices	4
1.1.1 Types of Warning Notices	
1.1.2 Structure of Warning Notices	4
1.2 Instructions	
1.3 Lists	
1.4 Symbols on the Package	
1.5 Symbols and Labels on mattress	5
1.6 Serial Labels	
1.6.1 Mattress Serial Label	
1.6.2 Mattress Wash Label	
1.7Abbreviations	
1.8 Definitions	
2 Safety Instructions	
2.1 Safety Instructions	
3 Intended use	
3.1 User population	
3.2 Contraindications	
3.3 Operator	
4Re-use	
5 Description of Mattresses	14
5.1 Correct Mattress Orientation	15
5.2 Transport Handles	17
6 Technical Specification	18
7 Use and Storage Conditions	19
8 Scope of Delivery and Product Variants	20
8.1 Delivery	
8.2 Scope of Delivery	
8.3 Variants	
9 Using the Mattress	21
9.1 Preparing the mattress for use	21
9.2 Rotating the mattress	
10Accessories and Replacement Components	22
11 Cleaning and Maintenance	23
11.1 General Cleaning	
11.2 Mattress Inspection	
12 Disposal	
12.1 Environment Protection	
12.2 Disposal	
12.2.1 Within Europe	
12.2.2 Outside Europe	
13 Warranty	
14 Standards and Regulations	
140tanuarus anu Negurations	25



# **1 Symbols and Definitions**

# 1.1 Warning Notices

# 1.1.1 Types of Warning Notices

Warning notices are differentiated by the type of danger using the following key words:

- ► CAUTION warns about the risk of material damage.
- ► WARNING warns about the risk of physical injury.
- ▶ **DANGER** warns about the risk of fatal injury.

#### 1.1.2 Structure of Warning Notices



SIGNAL WORDS!
Type and source of danger!
► Measures to avoid the danger.

#### 1.2 Instructions

#### Structure of instructions:

► Perform this step. Results, if necessary.

#### 1.3 Lists

#### Structure of bulleted lists:

- List level 1
  - □ List level 2
    - List level 3

# 1.4 Symbols on the Package

	KEEP DRY (PROTECT FROM HUMIDITY)
	TEEL DIST (FROTEOT FROM HOMEDITT)
LDPE	LOW DENSITY POLYETHYLENE RECYCLING SYMBOL
	RECYCLING SYMBOL



# 1.5 Symbols and Labels on mattress

	READ INSTRUCTIONS FOR USE
	DO NOT IRON
PHENOL	DO NOT USE A CLEANER CONTAINING PHENOL
	DO NOT WRING!
?	REGULARLY INSPECT THE INSIDE OF THE COVER FOR CONTAMINATION
71°	MACHINE WASH AT 71°C WITH DETERGENT
$\odot$	TUMBLE DRY ON LOW HEAT SETTING (MAX. 60°C)
H <sub>2</sub> O +	RINSE WITH WARM WATER AND NEUTRAL DETERGENT (INITIAL TEMPERATURE OF HOT WATER SHOULD NOT EXCEED 50°C)
NaCIO ≤1,000ppm	DISINFECT USING SOLUTION NO GREATER THAN 1,000PPM OF CHLORINE (SEE CHAPTER 'CLEANING AND MAINTENANCE')
H <sub>2</sub> O	RINSE WITH WARM WATER



6

BS 7175  S O O O O O O O O O O O O O O O O O O	MATTRESS CONFORMS TO BS7177:2008 FOR MEDIUM HAZARD
CE	CE MARK OF CONFORMITY WITH EU REGULATION
1	SYMBOL FOR TURNING AND ROTATING THE MATTRESS (SEE CHAPTER 'USING THE MATTRESS')
	DO NOT BLEACH
<u>P</u>	PROFESSIONAL CHEMICAL CLEANING (MODERATE PROCEDURE)
	MANUFACTURER
MD	MEDICAL DEVICE (compatible with Medical Device Regulation)
	GENERAL WARNING SIGN



# 1.6 Serial Labels

Pictures of serial labels below serve just for explanation of the signs and fields on the serial labels.

#### 1.6.1 Mattress Serial Label

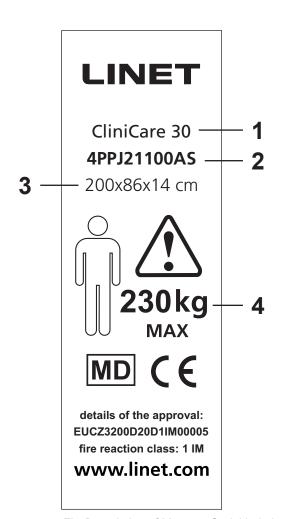


Fig. Description	of M	lattress	Serial	Label
------------------	------	----------	--------	-------

1	Mattress name (one name for different configurations)
2	Reference number depending on configuration
3	Mattress dimensions depending on configuration
4	Maximum Load



# LINET

EffectaCare 20 **4PPB21100AS** 

200x86x14 cm



MD (E

details of the approval: EUCZ3200D20D1IM00002 fire reaction class: 1 IM

www.linet.com

Fig. Mattress Serial Label for EffectaCare 20

# LINET

PrimaCare 20 B 4PPEB1100AS

200x100x16 cm



MD (E

details of the approval: EUCZ3200D20D1IM00003 fire reaction class: 1 IM

www.linet.com

Fig. Mattress Serial Label for EffectaCare 20 B (Bariatric)

### LINET

EffectaCare 20 P
4PPLI1100AS

137x70x10 cm



MD ( E

details of the approval: EUCZ3200D20D1IM00002 fire reaction class: 1 IM

www.linet.com

Fig. Mattress Serial Label for EffectaCare 20 P (Paediatric)

# LINET

PrimaCare 10 **4PPD21100AS** 

200x86x14 cm



<u>MD</u> ( (

details of the approval: EUCZ3200D20D1IM00001 fire reaction class: 1 IM

www.linet.com

Fig. Mattress Serial Label for PrimaCare 10

# LINET

PrimaCare 20 **4PPE21100AS** 

200x86x14 cm



MD (

details of the approval: EUCZ3200D20D1IM00003 fire reaction class: 1 IM

www.linet.com

Fig. Mattress Serial Label for PrimaCare 20

# LINET

PrimaCare 20 B 4PPEB1100AS

200x100x16 cm



MD (E

details of the approval: EUCZ3200D20D1IM00003 fire reaction class: 1 IM

www.linet.com

Fig. Mattress Serial Label for PrimaCare 20 B (Bariatric)





Fig. Mattress Serial Label for CliniCare 10

# CliniCare 10 P 4PPKI1100AS 137x70x10 cm 72 kg MAX MD C E details of the approval: EUCZ3200D20D1IM00004 fire reaction class: 1 IM www.linet.com

Fig. Mattress Serial Label for CliniCare 10 P (Paediatric)




Fig. Mattress Serial Label for CliniCare 20



Fig. Mattress Serial Label for CliniCare 30



# 1.6.2 Mattress Wash Label

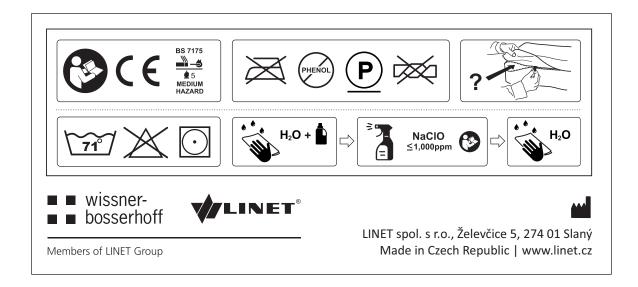

# 1.7 Abbreviations

В	Bariatric (mattress)
CE	European Conformity
CMHR	Combustion Modified High Resilience
CPR	Cardiopulmonary Resuscitation
ICU	Intensive Care Unit
IP	Ingress Protection
IV	Intravenous
MD	Medical Device
ME	Medical Electrical (Equipment)
Р	Paediatric (mattress)
PCM	Phase Change Material
ppm	parts per million, millionth (1000 ppm = 0,1%)
REF	Reference Number (product type depending on configuration)
SN	Serial Number
SWL	Safe Working Load
PU	Polyurethane
LDPE	Low Density Polyethylene

# 1.8 Definitions

Maximum Patient Weight on the bed with mattress	Maximum Patient Weight depends on the application environment according to IEC 60601-2-52. For application environment 1 (intensive/critical care) and 2 (acute care) reduce Safe working Load by 65 kg. For application environment 3 (long-term care) and 5 (ambulatory care) reduce Safe working Load by 35 kg.		
Maximum Load	he highest allowable load on the mattress.		
Adult	Patient having a physical size equal to or more than 146 cm, a mass equal to or more than 40 kg and a body mass index (BMI) equal to or more than 17 (according to IEC 60601-2-52).		
Child	Patient having a physical size equal to or less than 155 cm and a mass equal to or less than 70 kg.		



# **2 Safety Instructions**



#### **WARNING!**

These instructions for use MUST be given to the user of the product BEFORE using this product. Please read these instructions for use and save for future reference.



#### **WARNING!**

Do not use these products or any additional equipment without reading and understanding these instructions for use and any other instruction provided!



#### **WARNING!**

Any serious incident that has occurred in relation to the device should be reported to the manufacturer and the competent authority of the Member State in which the user and/or patient is established!



#### Warning!

This medical device is not intended for oxygen enriched environment!



#### **WARNING!**

This medical device is not intended for use with flammable substances!



#### WARNING!

This medical device is not portable medical electrical equipment!



#### **WARNING!**

Limited patient handling leads to development of pressure injury!



#### **WARNING!**

Before placing a patient on mattress, always have a suitably clinically qualified person perform a risk assessment to ensure that the support provided is appropriate and fulfils the local stipulations!



#### WARNING!

Support surface selection should be based on documented clinical reasoning, taking into consideration factors of the individual patient, e.g. mobility, heat, moisture, comfort etc.



#### WARNING!

High specification support surfaces are designed to complement, rather than replace, best practice in nursing care, e.g. regular patient turning.



#### WARNING!

Only nursing personnel trained according to the instructions for use is authorised to perform the installation of the mattresses on a compatible mattress support platform.



# 2.1 Safety Instructions

- ▶ It is necessary to read the instructions for use before using the mattress and perform maintenance according to the instructions for use.
- Follow the instructions carefully.
- Do not use a damaged mattress.
- If possible, check the mattress daily or between changing patients.
- Before positioning the patient the user must verify the condition of the mattress.
- Single sided mattresses are only to be used with the screen printing uppermost, and, if necessary, to check the mattress core has the profiling uppermost.
- The mattress must not be used if failures have been found that can do harm to the patient or mattress.
- The selection of the correct mattress type and application of the mattress must always be consulted with qualified clinical professional, especially in the case of an injury of the head, spinal cord or backbone.
- A patient with the indication of a higher risk of pressure ulcers than the mattress is designed for must not be placed on the mattress.
- It is necessary to monitor the condition of the patient and his/hers skin continuously and to change his/hers position on the mattress to prevent stressing risk and affected parts of his/hers body.
- The mattress must not be laid on the mattress platform if there is a danger the mattress could be disturbed or the cover torn with sharp parts of the bed or other sharp objects.
- During using of the mattress it is necessary to monitor the condition of the mattress core to ensure that it is not permanently compressed which will reduce the anti-decubitus properties of the product.
- Prolonged exposure of light can change the color tone of the mattress core. This change has no effect on physical properties of the mattress core. Polyurethane foams can have different colours. This has no effect on physical properties of the mattress core.
- The mattress cover may shrink slightly or its colour may fade. The mattress is still suitable for use provided the cover does not become a very tight fit (i.e can still bend under gentle pressure) and shows no signs of damage to the top coating.
- The mattress is equipped with PU cover and must not be covered with an additional waterproof sheet as this will stop its moisture vapour permability function of mattress cover.
- Do not put the bed into Trendelenburg or Anti-Trendelenburg position, when the head board and/or foot board are removed unless the bed frame is fitted with a retaining method to prevent the mattress from sliding up/down the bed when it is at such angles.
- The mattress must be placed on suitable type of mattress support platform according to the size of gaps between parts of mattress platform, which should not exceed 4 cm.
- The mattress must respect safety siderail height of a compatible medical bed.
- ▶ If the mattress platform has not features to provide ventilation to the base of the mattress, then the mattress should be regularly lifted and the base allowed to dry/breath before further use. This will prevent moisture damage to the base cover and extend the life of the mattress.
- Continually loaded mattress has shorter lifetime period.



#### 3 Intended use

The intended use of the EffectaCare 20, EffectaCare 20 B, EffectaCare 20 P, PrimaCare 10, PrimaCare 20, PrimaCare 20 B, CliniCare 10, CliniCare 10 P, CliniCare 20 and CliniCare 30 mattresses is to assist in the prevention of pressure ulcers. EffectaCare 20, EffectaCare 20 B and EffectaCare 20 P mattresses are intended for no more than medium risk of pressure ulcers creation.

PrimaCare 10, PrimaCare 20 and PrimaCare 20 B mattresses are intended for no more than high risk of pressure ulcers creation.

CliniCare 10, CliniCare 10 P, CliniCare 20 and CliniCare 30 mattresses are intended for no more than very high risk of pressure ulcers creation.

### 3.1 User population

- ► (Standard no code) Adult patients (weight >= 40 kg, height >= 146 cm, BMI >= 17)
- (Paediatric code P) Paediatric patients from age of 3 years (10 kg <= patient weight =< 75kg)
- (Bariatric code B) Bariatric patients (patient weight =< 250kg)</p>
- Caregivers (nurses, doctors, technical personnel, transport personnel, cleaning personnel)

#### 3.2 Contraindications

Patient with higher risk of pressure ulcers than the mattress is designed for:

- patients with higher weight than mattress weight limit
- patient's showing signs of pressure related tissue damage should be transferred onto an alternative support surface based on risk assessment, clinical reasoning and best clinical practice (EPUAP, NPUAP guidelines)
- Limited patient handling leads to development of pressure injury!

# 3.3 Operator

Caregiver

# 4Re-use

This product is suitable for repeated use. Before repeated use, ensure that the product is cleaned as per the cleaning and care instructions in these instructions for use.



# **5 Description of Mattresses**

These mattresses are designed to be used in conjunction with a suitably sized mattress support platform, and as part of a pressure ulcer prevention care programme. These mattresses are not designed for any other use and any such use would void the manufacturer's warranty. These mattresses have been designed to deliver effective pressure re-distribution when used in accordance with the instructions in the instructions for use.

	Mattress Type					
Mattress Feature	EffectaCare 20	EffectaCare 20 B (Bariatric)	EffectaCare 20 P (Paediatric)	PrimaCare 10		
High resilience foam base	~	~	~	<b>~</b>		
Supporting side walls						
High resilient foam topper						
Visco-elastic (memory foam) topper						
PCM top layer						
Machine-hinged profiling	<b>✓</b>	<b>✓</b>	<b>✓</b>	<b>✓</b>		
Single sided	<b>✓</b>	<b>✓</b>	<b>✓</b>	<b>✓</b>		
Rotate only design	<b>→</b>	<b>✓</b>	~	<b>✓</b>		
Welded cover seams	<b>✓</b>	<b>✓</b>	<b>✓</b>	<b>✓</b>		
180° degree zip	<b>✓</b>	~	<b>✓</b>	<b>~</b>		
Maximum Load	150kg	300kg	72kg	200kg		

	Mattress Type					
Mattress Feature	PrimaCare 20	PrimaCare 20 B (Bariatric)	CliniCare 10	CliniCare 10 P (Paediatric)	CliniCare 20	CliniCare 30
High resilience foam base	~	<b>&gt;</b>	<b>~</b>	~	<b>&gt;</b>	<b>~</b>
Supporting side walls			<b>~</b>		<b>&gt;</b>	<b>~</b>
High resilient foam topper	~	<b>&gt;</b>				
Visco-elastic (memory foam) topper			~	~	>	~
PCM top layer						<b>✓</b>
Machine-hinged profiling	<b>✓</b>	<b>&gt;</b>	<b>&gt;</b>	<b>✓</b>	<b>&gt;</b>	<b>~</b>
Single sided	<b>✓</b>		<b>~</b>	~	<b>✓</b>	<b>~</b>
Rotate only design	<b>✓</b>	<b>~</b>	<b>~</b>	~	<b>✓</b>	<b>&gt;</b>
Welded cover seams	~	<b>~</b>	<b>~</b>	~	<b>~</b>	<b>&gt;</b>
180º degree zip	<b>✓</b>	<b>~</b>	~	~	<b>&gt;</b>	~
Maximum Load	200kg	300kg	200kg	72kg	230kg	230kg



#### **5.1 Correct Mattress Orientation**




Fig. EffectaCare 20 (side view)

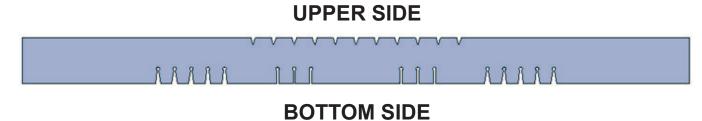


Fig. EffectaCare 20 B (side view)



Fig. EffectaCare 20 P (side view)

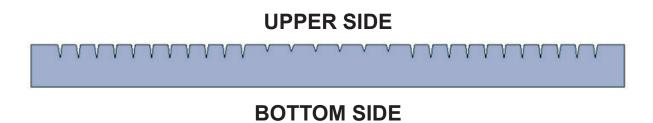


Fig. PrimaCare 10 (side view)




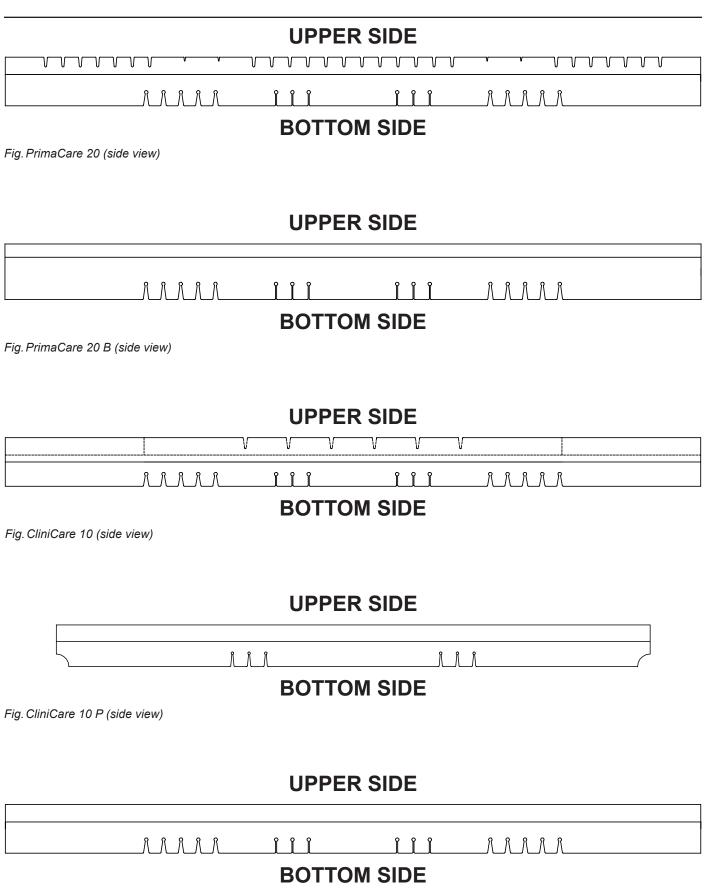


Fig. CliniCare 20 (side view)



#### **UPPER SIDE**



# **BOTTOM SIDE**

Fig. CliniCare 30 (side view)

# **5.2 Transport Handles**



#### **WARNING!**

Material damage and risk of injury due to incorrect use!

► Transport the mattress using transport handles without patient on it!

Transport handles are intended for transport of the PrimaCare 20, PrimaCare 20 B, CliniCare 10, CliniCare 10 P, CliniCare 20 and CliniCare 30 mattresses.



Fig. Transport Handles on the Cover



# **6 Technical Specification**



#### **WARNING!**

If these mattresses are used with any compatible medical bed, respect values of mechanical specifications which can harm neither mattress nor medical bed!

	EffectaCare Range			
	EffectaCare 20	EffectaCare 20 B (Bariatric)	EffectaCare 20 P (Paediatric)	
Mattress type	Preventive anti-decubitus	Preventive anti-decubitus	Preventive anti-decubitus	
Material of foam	Polyurethane foam	Polyurethane foam	Polyurethane foam	
Material of cover Backing Coating	100% polyester 100% polyurethane			
Cover	Water resistant and vapour permeable See Cleaning and Maintenance for additional information			
Weight of mattress	8kg	15kg	3,5kg	
Height of mattress	14cm	16cm	10cm	
Risk of pressure ulcers creation	Medium risk*	Medium risk*	Medium risk*	
Warranty	1 year**	1 year**	1 year**	
Stacking limit	15 pieces	15 pieces	25 pieces	

<sup>\*</sup>Indication of use based upon interface pressure readings – not a prescriptive criteria. Always refer to a clinician's judgement.

<sup>\*\*</sup>In accordance with an appropriate turning and repositioning regime and with the proper usage and cleaning instructions (see Cleaning and Maintenance chapter).

	PrimaCare Range				
	PrimaCare 10	PrimaCare 20 B (Bariatric)			
Mattress type	Preventive anti-decubitus	Preventive anti-decubitus	Preventive anti-decubitus		
Material of foam	Polyurethane foam	Polyurethane foam	Polyurethane foam		
Material of cover Backing Coating	100% polyester 100% polyurethane				
Cover	Water resistant and vapour permeable See Cleaning and Maintenance for additional information				
Weight of mattress	10kg	11kg	14kg		
Height of mattress	14cm	14cm 14cm 16cm			
Risk of pressure ulcers creation	High risk* High risk* High risk*				
Warranty	2 years**	2 years**	2 years**		
Stacking limit	15 pieces	15 pieces	15 pieces		

<sup>\*</sup>Indication of use based upon interface pressure readings – not a prescriptive criteria. Always refer to a clinician's judgement.

<sup>\*\*</sup>In accordance with an appropriate turning and repositioning regime and with the proper usage and cleaning instructions (see Cleaning and Maintenance chapter).



	CliniCare Range			
	CliniCare 10	CliniCare 10 P (Pae- diatric)	CliniCare 20	CliniCare 30
Mattress type	Preventive anti-decu- bitus	Preventive anti-decubitus	Preventive anti-decubitus	Preventive anti-decu- bitus
Material of foam	Polyurethane foam, visco-elastic foam	Polyurethane foam, visco-elastic foam	Polyurethane foam, visco-elastic foam	Polyurethane foam, visco-elastic foam, PCM layer
Material of cover Backing Coating	100% polyester 100% polyurethane			
Cover	Water resistant and vapour permeable See Cleaning and Maintenance for additional information			
Weight of mattress	13kg	6kg	16kg	13kg
Height of mattress	14cm	10cm	14cm	14cm
Risk of pressure ul- cers creation	Very high risk*	Very high risk*	Very high risk*	Very high risk*
Warranty	2 years**	2 years**	2 years**	2 years**
Stacking limit	15 pieces	25 pieces	15 pieces	15 pieces

<sup>\*</sup>Indication of use based upon interface pressure readings – not a prescriptive criteria. Always refer to a clinician's judgement.

\*\*In accordance with an appropriate turning and repositioning regime and with the proper usage and cleaning instructions (see Cleaning and Maintenance chapter).

# **7Use and Storage Conditions**

Respect values of the parameters connected with environment conditions in the chapter Technical Specification during use and storage of the product.

EffectaCare 20, EffectaCare 20 B, EffectaCare 20 P, PrimaCare 10, PrimaCare 20, PrimaCare 20 B, CliniCare 10 P, CliniCare 20 and CliniCare 30 mattresses are not suitable for indoor environments containing flammable gases (except oxygen cylinders).

EffectaCare 20, EffectaCare 20 B, EffectaCare 20 P, PrimaCare 10, PrimaCare 20, PrimaCare 20 B, CliniCare 10 P, CliniCare 20 and CliniCare 30 mattresses are suitable for continuous operation.

#### When mattress is not in use:

- Store the mattress flat.
- Do not fold the mattress.
- Do not place heavy objects on the mattress surface when not in use.
- Do not allow sharp objects to penetrate the cover coating.
- Keep the mattress clean.
- Regularly inspect the exterior of the mattress.
- ▶ Do not store in damp conditions.
- When removing packaging use great care to ensure the cover is not damaged.

D9U004PPM-0101 01 19



# **8 Scope of Delivery and Product Variants**

# 8.1 Delivery

- Upon receipt, check that the shipment is complete as specified on the delivery note.
- Notify the carrier and supplier of any deficiencies or damages immediately as well as in writing or make a note on the delivery note.

# 8.2 Scope of Delivery

- Mattress
- Instructions for use

#### 8.3 Variants

- EffectaCare 20
- EffectaCare 20 B
- EffectaCare 20 P
- PrimaCare 10
- PrimaCare 20
- PrimaCare 20 B (Bariatric)
- CliniCare 10
- CliniCare 10 P (Paediatric)
- CliniCare 20
- CliniCare 30

20



# 9 Using the Mattress



#### **DANGER!**

Risk of suffocation due to air-impermeable mattress cover!

- Use mattress cover correctly.
- ► The nursing staff are responsible for the safety of the patient on the mattress cover!



#### WARNING

Always consider shape and dimensions of the mattress platform for which the mattress will be used.



#### **WARNING!**

Ensure that the surface of the bed is clear from debris before placing the mattress – debris can damage the coating of the fabric.



#### WARNING!

Always ensure where is the upper side and bottom side of the mattress before putting the mattress cover back on the mattress foam core!



#### WARNING!

Never manipulate with mattress by grabbing it by its seams. This may cause damaging the mattress cover and risk of fluids penetrating into the mattress core!



#### **CAUTION!**

Material damage due to dampness or contamination!

▶ Make sure mattress cover has been cleaned and is completely dry.

#### 9.1 Preparing the mattress for use

- Ensure that all packaging is removed from the mattress before use
- Lay the mattress flat on to the frame of the bed
- For a rolled mattress, lay the mattress flat and allow at least an hour for the mattress to restore to its original shape.
- Ensure the mattress is dry before use

# 9.2 Rotating the mattress

The LINET PrimaCare and CliniCare products detailed in this manual are single-sided. Single-sided mattresses have numbers 1 and 2 on the top surface and can only be rotated, not turned (refer to the picture below for demonstration)

When replacing the mattress cover on a single-sided mattress, make sure that the protective flap on the cover zip is correctly positioned to prevent fluid ingress.

Frequent rotation is strongly recommended for non-turn mattresses as all foam grades fatigue during use and rotating will ensure loading is evenly spread across both ends of the mattress. Recommended interval of rotating/turning is once a month. When rotating a mattress, always grab the mattress from bottom side. Never manipulate with mattress by grabbing it by its seams. This may damage the cover and increase the risk of fluid ingress entering via the zip.

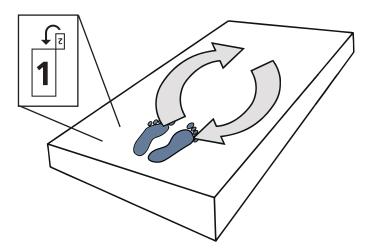


Fig. Rotation of mattress and screen print symbol



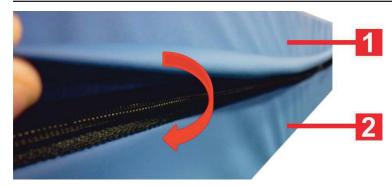


Fig. Correct placement of the top cover flap

- 1. Top cover
- 2. Base cover

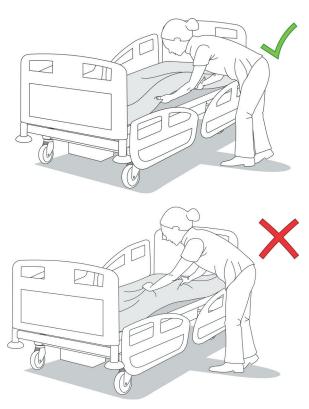


Fig. Manipulation with mattress

# 10 Accessories and Replacement Components

#### **Extensions, Foams and Covers**

There is a selection of mattress extensions available where necessary. Suitability of extension will be dependent on application and mattress type. Three styles of extension are available:

- Standard (CMHR foam layers)
- Comfort (CMHR base with a visco layer top)
- Bariatric (High durability CMHR foam layers)

Replacement foam and covers are available where necessary. For more information on the following items please contact your local LINET distributor.



# 11 Cleaning and Maintenance



#### **WARNING!**

The cover fabric is treated with biocide against bacteria and fungi. This antibacterial agent reduces effectively the development of bacteria. The active biocide substance is zinc pyrithione.



#### **WARNING!**

The following instructions apply to the cleaning and maintenance of the cover only. The foam construction must not be disinfected or laundered as this will affect the integrity of the mattress.



#### **WARNING!**

It is recommended to clean this product with water and soap only. Cleaning products containing alcohol, solvent, bleach or abrasive products can damage this product.

## 11.1 General Cleaning

For general cleaning and superficial dirt, use a disposable wipe with a solution of warm water and neutral detergent. Do not use abrasive or phenolic-based cleaners. Cleaning by neutral water and soap, followed by rinsing with water, is sufficient to clean this product. Solvent containing alcohol, bleaching or abrasive products can be harmful. On request, the manufacturer will provide list of cleaning agents and disinfectants tested with the mattresses.

To disinfect in situ, use a 0.1% sodium hypochlorite solution (1,000ppm chlorine). If required, a 1% chlorine solution (10,000ppm) and cold water may be applied for no more than 2 minutes. Thoroughly rinse the cover with clean water and allow drying before re-use or storage.

Removable, contaminated covers should be laundered at 71°C for no more than 10 minutes or at 95°C for no more than 3 minutes. Spin and tumble dry at no more than 60°C. Do not mangle or iron.

# 11.2 Mattress Inspection

- Check the mattress for signs of tearing and/or punctures.
- 2. Check the seams for any signs of splitting.
- 3. Check the zip(s) if applicable for any signs of damage.
- 4. Check for any signs of permanent staining.



# 12 Disposal

#### 12.1 Environment Protection

The company LINET® is aware of the importance of environmental protection for future generations. Within this company the environmental management system is applied in accordance with the internationally agreed standard ISO 14001. The compliance with this standard is annually tested by the external audit executed by an authorised company. Materials used in this product are not environmentally hazardous. LINET® products meet valid requirements of national and European legislation in the areas of **RoHS** and **REACH**, so they do not contain any prohibited substances in excess quantities. None of the wooden parts is made of tropical wood (such as mahogany, rosewood, ebony, teak etc.) or made of timber from the Amazon region or from similar rainforests. Used packaging materials are in accordance with requirements of the Packaging Act (**Zákon o obalech**). For disposal of packaging materials after installation of products contact your sales representative or manufacturer's customer service about the possibility of a free take-back of packaging through an authorized company (more details on **www.linet.cz**).

#### 12.2 Disposal

#### 12.2.1 Within Europe

#### To dispose of the mattress:

- ▶ Ensure that the mattress is fully decontaminated prior to disposal.
- ▶ The equipment must not be disposed of as household waste.
- Dispose of this equipment at designated collection points or take-back points.

LINET® participates in a collective system with take-back company REMA System (see **www.remasystem.cz/sberna-mista/**). By bringing electric and electronic equipment to a take-back point, you participate in recycling and you save primary raw material resources while protecting your environment from effects of unprofessional disposal.

#### 12.2.2 Outside Europe

#### To dispose of the mattress:

- ► Ensure that the mattress is fully decontaminated prior to disposal.
- Dispose of the product or its components in accordance with local laws and regulations!
- Hire an approved waste disposal company for disposal!



# 13 Warranty

The EffectaCare, PrimaCare and CliniCare mattress ranges are covered against faulty manufacture and materials as replacement goods. The length of warranty for each type of mattress is stated in chapter Technical Specification.

Normal wear and tear expected would not be included.

All warranties subject to LINET terms and conditions of trading.

In order to claim under warranty refer to the batch number printed on the product label. Never remove the label.

If a defect or fault is discovered, the LINET representative from whom the product was obtained must be notified immediately. For potentially serious and/or life-threatening situations, your local Competent Authority must be informed.

# 14 Standards and Regulations

Apllied norms are stated on Declaration of Conformity.

The manufacturer adheres to a certified quality management system in compliance with the following standards:

- ISO 9001
- ISO 14001
- ISO 13485
- MDSAP (Medical Device Single Audit Program)

All LINET EffectaCare, PrimaCare and CliniCare mattresses are considered as medical devices, and therefore feature the CE mark, in accordance with EU Medical Device Regulation 2017/745.

Manufacturer is committed to advancing responsible care, continuously improving environmental, health and safety knowledge and the performance of used technologies, processes and products over their lifecycles. As a result, only REACH compliant materials and components are used.

The foam and cover used to manufacture the LINET EffectaCare, PrimaCare and CliniCare ranges of mattresses are independently tested and are certified in accordance with EN597-1 and EN597-2 (Assessment of the ignitability of mattresses and upholstered bed bases – ignition source: smouldering cigarette (1) and match flame equivalent (2)).

Each product is individually tested as a composite in accordance with BS7177 ignition sources 0,1 and crib 5.

For further information on standards and regulations, please contact your LINET representative.